


OxyPro-XT

User Manual

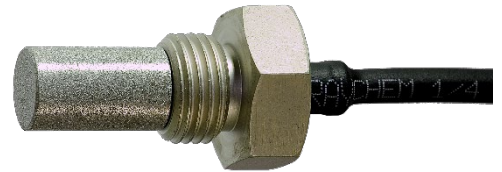

Revision History

Issue No.	Description	Date	Author Initials
00	New document	09/2025	PS



SENSORE Electronic GmbH
Aufeldgasse 37-39
A-3400 Klosterneuburg
Austria

For contact information, visit
sensore-electronic.com

SENSORE Electronic GmbH is part of the DwyerOmega group.
This document is the property of SENSORE Electronic GmbH. and may not be copied or otherwise reproduced,
communicated to third parties, nor stored in any Data Processing System without the express written authorization of SENSORE
Electronic.

© 2025 SENSORE Electronic GmbH
SENSORE, a DwyerOmega brand

Before using your OxyPro-XT

The OxyPro-XT is a one channel system, some illustrations in the user manual will be based on the OxyPro-XT2 the dual channel version, in such a case the 2nd channel can be ignored.

Safety Information



Necessary safety precautions are described in the following chapters and also highlighted using pictographic warnings on yellow background (as above).

The OxyPro-XT must not be used for safety critical applications.

For integration into a larger system, the system developer must ensure the correct installation according to this manual and verify the sensor function under application conditions. Installation, initial commissioning, inspection, maintenance, and servicing must be carried out by trained specialists.

Abbreviations

AC	Alternating Current
AM	Additive Manufacturing
Ar	Argon
CO ₂	Carbon Dioxide
DC	Direct Current
°C	Degrees Celsius
°F	Degrees Fahrenheit
EEPROM	Electrically Erasable Programmable Read-only Memory
ESD	Electrostatic Discharge
g	Grams
GND	Ground
kg	Kilogram
LED	Light Emitting Diode
mA	Milliamp
N ₂	Nitrogen
PPM	Parts per Million
PELV	Protective Extra Low Voltage
SELV	Safety Extra Low Voltage
ZrO ₂	Zirconium Dioxide

Contents

Revision History	i
Before using your OxyPro-XT	ii
Safety Information	ii
Abbreviations	ii
1 Introduction	1
1.1 Scope of Use	1
1.2 Feature Overview	2
1.3 System Overview based on the two-channel version OxyPro-XT2	3
2 OxyPro-XT Oxygen Monitoring Functions	4
2.1 O ₂ Threshold Detection (Alarm Levels)	4
2.2 Analog Output (4...19mA) with special conditions (19...20mA)	4
2.3 Further analog output options (0...5 V, 4...20 mA)	5
2.4 Digital Output (RS485/Modbus)	5
2.5 Status LEDs/System States	5
3 Installation	6
3.1 Sensor Installation in a Process Chamber	6
3.2 Connection in a Control Cabinet based on OxyPro-XT2	7
3.3 Sensor Connection	9
3.4 Route Cables and Shielding Grounding	10
4 Commissioning	11
4.1 Initial Power-up	11
4.2 Power-up after Maintenance	11
4.3 Decommissioning	11
4.4 Recommissioning	11
4.5 System Behavior During Commissioning	11
5 Maintenance	12
5.1 Inspect Your Sensors/Sensor Cleaning	12
5.2 Inspect Your OxyPro-XT – Basic Function Test	12
5.3 Process Measurement Accuracy	12
6 Repairs and Replacements	13
6.1 Replace the Sensor	13
6.2 Replace the OxyPro-XT transmitter	13
6.3 Installation Changes	13
7 Disposal and Recycling	14
8 Troubleshooting	15
8.1 Error Codes	15
8.2 Recovering from (Permanent) Fault Conditions	16
8.3 Interference with O ₂ Measurement	16
9 RS485 Modbus Interface	17
9.1 RS485 Parameters	17

9.2 Modbus Functions	17
9.3 Modbus Communication Examples	18
9.4 Modbus Register Overview	19
9.5 Digital Status Register 16Bit (Modbus Register 0x0000)	21
9.6 Digital System States (Modbus Register 0x0016)	22
10 Appendices.....	23
Appendix A - Technical Specifications	23
Appendix B - Technical Drawings (mm)	24
Appendix C - Quality, Recycling, and Warranty Information	25

1 Introduction

The OxyPro-XT oxygen transmitter measures oxygen (O₂) by means of amperometric zirconium dioxide (ZrO₂) sensors where the volumetric O₂ concentration in gas mixtures is determined. The alarm relay contact will be switched based on a user programmable threshold value.

1.1 Scope of Use

OxyPro-XT is ideal for use in the following applications:

Laboratory / Measuring instrumentation:

- Oxygen meter
- Measurements under controlled O₂ content
- Inert gas processing cabinets (glove boxes)
- Incubators (controlled bacterial growth)

Food industry:

- Packaging and controlled food testing

Medical:

- Oxygen concentrators

Industry:

- Nitrogen/Oxygen concentrators
- Additive Manufacturing (AM)
- Inert gas processing machines and cabinets
- Inert gas welding monitoring
- Storage with increased N₂ atmosphere (oxidation prevention)
- Drying units

NOTE: The sensors are calibrated and specified for nitrogen balance gas. Argon can also be used as a balance gas; this will slightly affect the system accuracy.

Application limitations are listed below:

- The system must not be used in safety critical applications
- The system is not ATEX-approved because its internal sensor achieves elevated temperatures during normal use (up to ca. 600 °C)
- The use in deviating balance gases e.g. carbon dioxide (CO₂) is possible, but potential cross-sensitivities must be considered, please contact SENSORE for more information.
- The sensor is not recommended for use in flammable gases, as local combustion can cause inaccurate (reduced) O₂ concentration readings. If used in flammable gases, the concentration of combustible gases must be negligible to the O₂ concentration.
- The sensor is not suitable for measuring O₂ concentrations in liquids.
- The sensor is not suitable for use with AM plastic powders or filaments.
- The sensor is not suitable for conditions with condensing humidity, and therefore not suitable for outdoor use.

1.2 Feature Overview

- The current-limiting zirconia sensor ensures high accuracy over long-life.
- Smart Sensor with M12 connection
 - Sensor calibration and parameter data are stored in the memory chip of the sensor
 - Upon connection of the sensor the setup is uploaded to the OxyPro-XT transmitter
 - Available with various housing options and measurement ranges
 - Plug and play approach for easy sensor replacement in the end application
- OxyPro-XT transmitter
 - DIN rail mounting for installation inside a control cabinet.
 - Supply via external 24 V DC SELV (safety extra-low voltage) LPS (limited power supply), e.g. NEC Class 2 power supply.
 - Maximum current consumption: 250 mA
- Sensor control circuits
 - Active control of the sensor chip temperature, to compensate for external influences in a temperature range of +10...+100 °C (+50...+212 °F)
 - Sensor current limitation in case of overrange operation, to extend the sensor lifetime
- Diagnostic features to detect possible fault conditions, e.g.:
 - Detection of external wiring issues
 - Monitoring external supply voltage and the internal circuit temperature
- Several signal output options
 - digital: RS485 (Modbus)
 - analog: 4...20 mA output (recommended analog output option)
 - analog: 0...5 V output (fallback option)
 - potential-free relay contact
alarm level and switching directions can be programmed via RS485

1.3 System Overview based on the two-channel version OxyPro-XT2

For the one channel version OxyPro-XT please ignore the 2nd channel

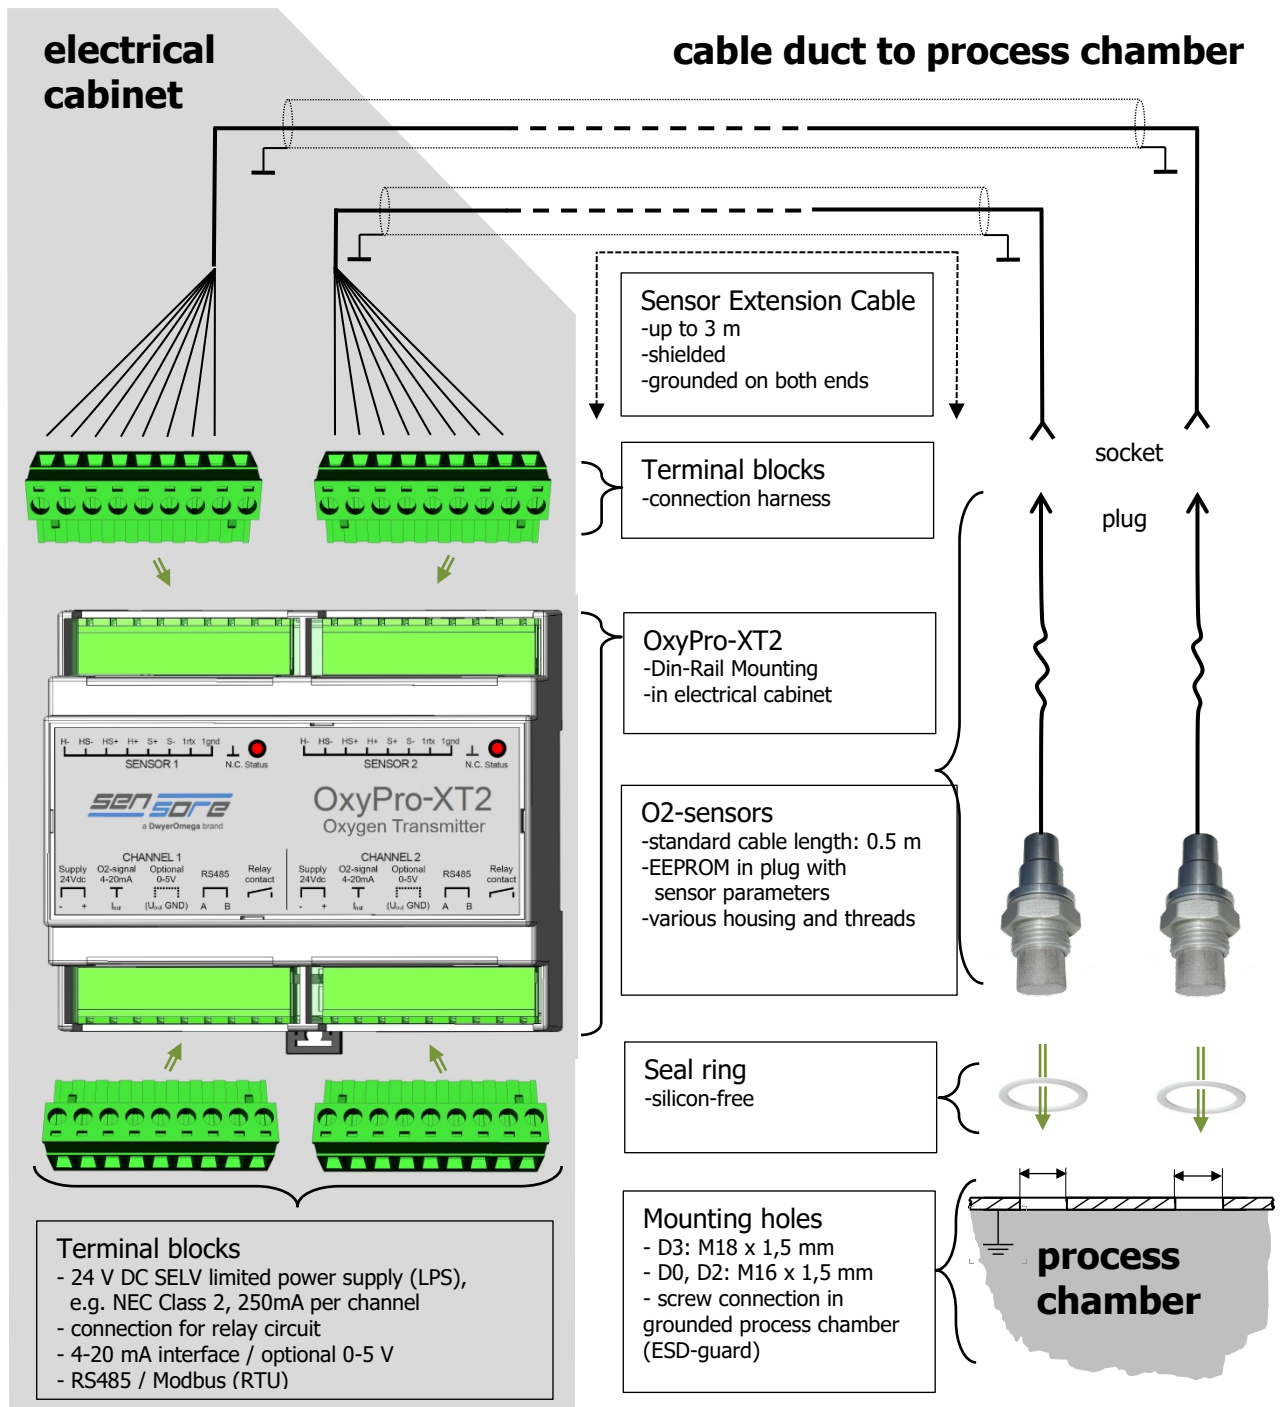


Figure 1. Larger System schematic

The specification for the O₂ measurement is determined by the sensor.

- The design of the sensor chip defines the O₂ measuring range.
- The calibration information is stored in the sensor connector (EEPROM).

2 OxyPro-XT Oxygen Monitoring Functions

The essential operating parameters for the sensors are in a non-volatile memory (EEPROM) on the sensor connector, i.e. there is no need to calibrate the sensors with or match them to a specific monitor.

2.1 O₂ Threshold Detection (Alarm Levels)

It is possible to program an O₂ threshold value to control the potential-free contact pair (relay). The switching direction defines if the relay will close on a rising edge or a falling edge. To avoid unnecessary switching a switching hysteresis must be defined. See section 9.4.4 on how to program the threshold levels / hysteresis via RS485/Modbus.

- Closing on falling edge
 - Activation threshold: If the O₂-signal falls below, the contacts will close
 - Deactivation threshold: If the O₂-signal rises above, the contacts will open
- Closing on rising edge
 - Activation threshold: If the O₂-signal rises above, the contacts will close
 - Deactivation threshold: If the O₂-signal falls below, the contacts will open

2.2 Analog Output (4...19mA) with special conditions (19...20mA)

The analog output configuration is a combination of analog O₂ signal output 4...19 mA and the analog indication of special conditions (19...20 mA). The table below summarizes the scaling of the 4...19 mA for different nominal sensor ranges. By using the digital RS 485 output it is possible to avoid the restrictions of the analog output.

Available measurement ranges		O ₂ concentration in volumetric % or ppm					
Nominal sensor range*	1000 ppm	1.00 %	2.00 %	5 %	25 %	40.0 %	96.0 %
Analog full scale (19mA)	1125 ppm	1.17 %	2.35 %	5.86 %	23.5 %	46.9 %	93.8 %
Option: Analog full scale (20mA/5V)	1200 ppm	1.25 %	2.5 %	6.25 %	25 %	50 %	100 %
usable digital range (RS 485)	1200 ppm	1.25 %	2.5%	6.25 %	25 %	50 %	100 %
Typical Accuracy	20 ppm	100 ppm	200 ppm	500 ppm	0.25 %	0.40 %	1.0 %
Output Resolution (4...19 mA)	< 1 ppm	< 10 ppm	< 20 ppm	< 50 ppm	< 0.025 %	< 0.04 %	<0.1 %
Lower Detection Limit	10 ppm	100 ppm	100 ppm	500 ppm	0.1 %	0.2 %	1.0 %

*Nominal sensor range is the specified maximal O₂ concentration, overrange operation should be avoided

Calculation:

$$\text{Measured } O_2 = \frac{I_{out} [mA] - 4mA}{15mA} \times \text{Analog full scale (19mA)}$$

- I_{out} is the measuring current of the 4...20 mA current loop
- The value range is cut off at 19 mA
- Current values between 19 and 20 mA are used to indicate special states and faults
- Special state indication:
 - 19.15 mA Heat up
 - ≥19.2 mA Error
 - ~0.5 mA Over-temperature shutdown (special fault mode).

2.3 Further analog output options (0...5 V, 4...20 mA)

Instead of using 4...19 mA for analog signal and using 19...20 mA for special conditions, it is also possible to use 4...20 mA for analog signal and > 20 mA for special conditions/errors, see also section 9.4.5 on how to change this via MODBUS or contact SENSORE to order a customized Smart Sensor.

The OxyPro-XT also features a 0...5 V output. To avoid ground loop issues, the 0...5 V should be connected to an isolated analog input. In case of special conditions or errors, the output will be 5 V.

Calculation:

$$\text{Measured } O_2 = \frac{I_{out} [mA] - 4mA}{16mA} \times \text{Analog full scale (20mA/5V)}$$

$$\text{Measured } O_2 = \frac{U_{out} [V]}{5V} \times \text{Analog full scale (20mA/5V)}$$

- I_{out} is the measuring current of the 4...20 mA current loop
- U_{out} is the measuring current of the 0...5 V voltage output

2.4 Digital Output (RS485/Modbus)

$$\text{Measured } O_2 = \frac{O_{2norm}}{1000} \times \text{usable digital range (RS 485)}$$

- The digital value "O₂norm" is read out via register 0x0002
- The digital value range is cut off at 1250, i.e. an O₂ measurement value is transmitted digitally even if the measuring range is slightly exceeded
- Special states can be read via registers 0x0000
- Further details on RS485/Modbus communication can be found in section 9.

2.5 Status LEDs/System States


Stable (Measurement) States	
LED permanently on	O ₂ measurement mode
Temporary States (during start-up)	
LED 0.5s on, 0.5s off	Contact check of the sensors (usually imperceptible 1...2 s)
LED 0.2s on, 0.8s off	Heating phase of the sensors (typically 60 s)
Error States that may resolve without intervention	
LED flashing (10 Hz)	Error mode (restart the sensor after 60s)
LED off	Temporary complete extinction of the LED, followed by failure mode, occurs when overtemperature protection mode is activated. => check installation situation / check ambient temperature
Error States that require intervention	
LED 0.5s on, 0.5s off	System gets stuck in contact test => check the connection of the sensors
LED flashing (10 Hz) longer than 60s	No reboot from error mode, after repeated error => see 8.2

3 Installation


Only assemble and install the transmitter when it is powered off and disconnected from the electricity supply.

3.1 Sensor Installation in a Process Chamber

- Silicone-free materials must be provided for sealing.
- The system has been evaluated for applications within gas temperatures ranging from 10...100 °C (50...212 °F). Monitoring oxygen at higher gas temperatures is feasible, but should be discussed with the application engineering team, please contact SENSORE.

 Positioning the sensors incorrectly in the process chamber can negatively impact measurement. To avoid this:

- Do not mount sensors in the immediate vicinity of gas inlets or outlets
- Do not place them near heaters/fans or in direct airflow
- Mount on surfaces that will not vibrate.

 For oxygen measurement, the gas must pass the sensor's porous sinter cap/disc or the inlet mesh. To facilitate this:

- The sinter cap/disc or the mesh should protrude into the process chamber as much as possible
- Contamination/encrustation of the sinter cap/disc or the inlet mesh must be avoided
- Mounting the sensor upside down should reduce contamination risks.

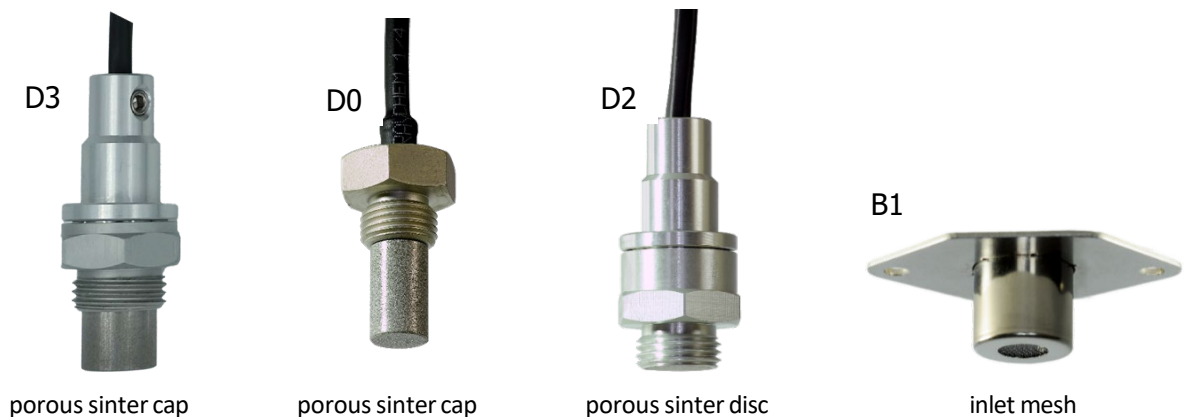


Figure 2. Sensor's porous sinter cap/disc or inlet mesh

 If the sensor is located so that its housing is easily accessible to end-users, please note the following:

- During operation, the sensor housing's temperature might exceed 60 °C (140 °F)
 - Sensor housing temperature depends on the selected sensor head design (Figure 2) and the thermal connection to the process chamber.
- Use appropriate warning labels, e.g. "hot surface"



- When the sensor's metal housing is screwed directly into the grounded metal wall of the process chamber, it provides adequate protection against electrostatic discharge (ESD). Refer to Figure 1 for guidance.

3.2 Connection in a Control Cabinet based on OxyPro-XT2

For the one channel version OxyPro-XT please ignore the 2nd channel

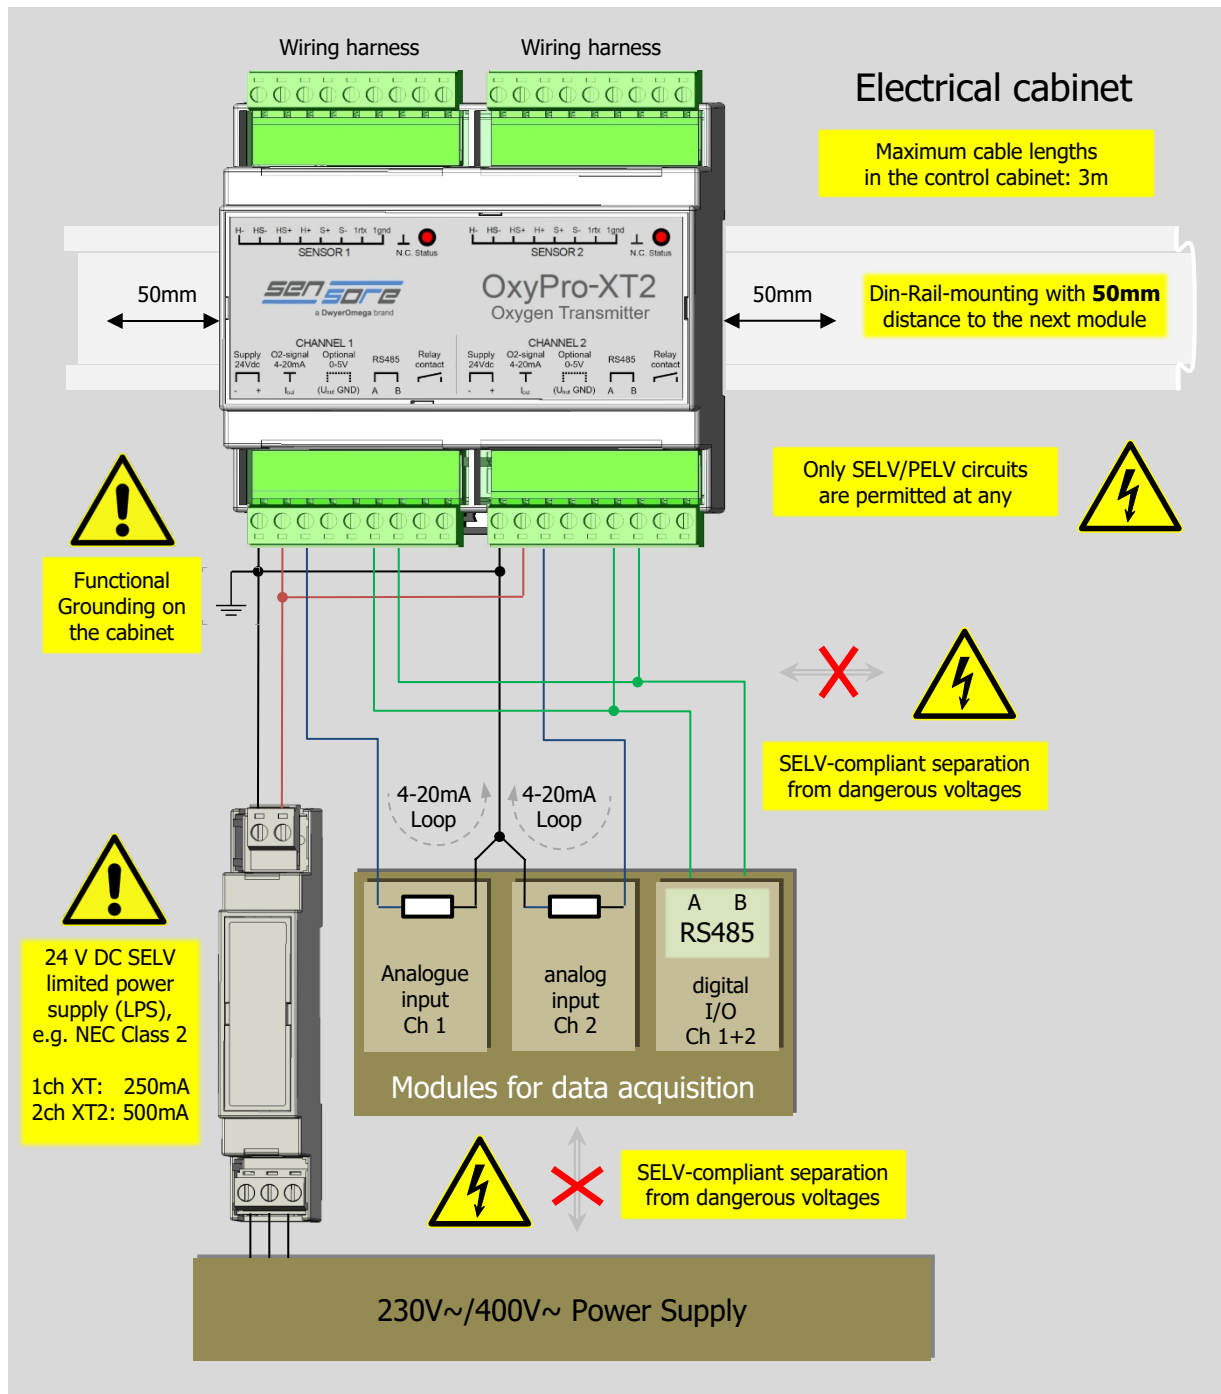


Figure 3. Control Cabinet Connections

NOTE: Installation must be carried out by trained specialists.

- OxyPro-XT can be mounted on a DIN rail in a control cabinet.
- Functional Grounding must take place at one point, in the immediate vicinity of the transmitter. Due to the grounding the resulting circuit will be PELV (Protective Extra Low Voltage)

3.2.1 Connection Assignment - Control Cabinet Side

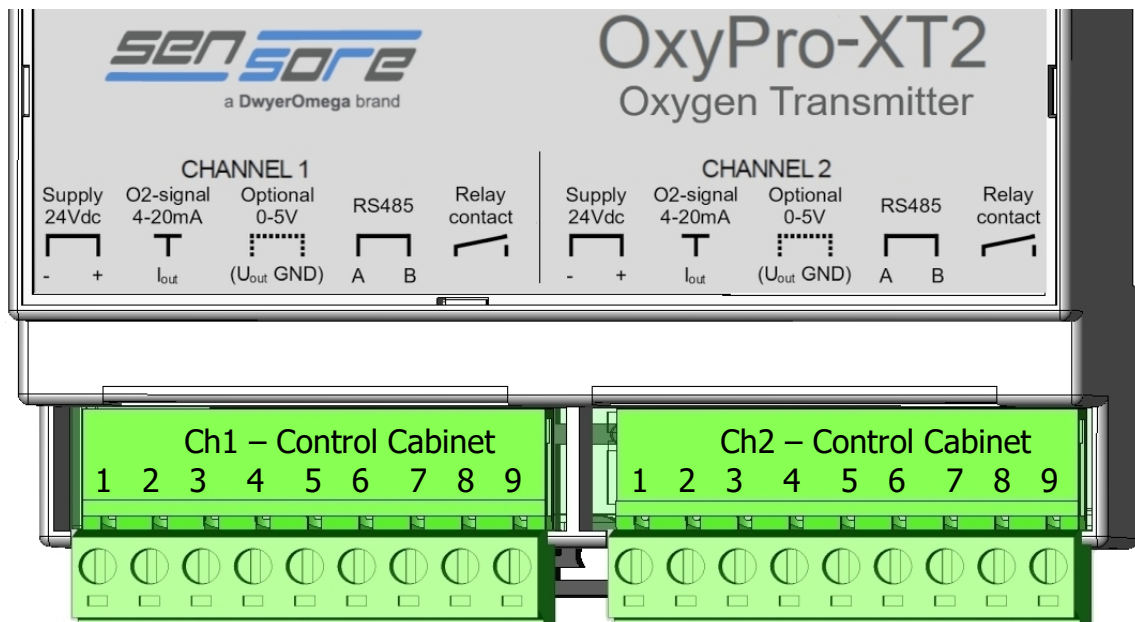


Figure 4. Cabinet side connections


POs	Function	Information
1	Power supply 24 V - (Earth)	To be connected to SELV power supply
2	Power supply 24 V +	
3	Iout (4...20 mA)	Current loop output for the O ₂ reading, must be traced back to pin 1 (see section 3.2)
4	Uout (0-5 V)	4...20 mA is the recommended analog output, using 0...5 V output might cause GND-loop issues. Use a high impedance differential input for 0...5 V signal.
5	GND (0-5 V)	
6	RS485 A	Connection to RS485 only SELV/PELV compliant circuits
7	RS485 B	
8	Relay contact/Potential free contact pair	Only SELV/PELV compliant circuits, rating 24Vdc / 100mA user configurable alarm levels
9		

- Optional voltage output 0...5 V, Uout and GND (pins 4 and 5).
It is recommended to use the 4...20 mA instead of 0...5 V to avoid the following issues:
 - The analog voltage output will not indicate certain faults (e.g. cable breakage, power loss).
A 0 V output due to a fault condition might be falsely interpreted as 0% O₂.
 - The analog voltage output could create GND-loop issues
- RS485
 - Ground reference for the RS485 signals is pin 1. This means that a possible RS485 ground connection must be made to pin 1 (not pin 5)

3.2.2 Wire the Sensors

The electronics and sensors are connected to each other via cable harnesses, permanently installed in the system. These along with short sensor cables (50 cm), facilitate easy sensor installation.

3.2.3 Connection Assignment - Sensor Side

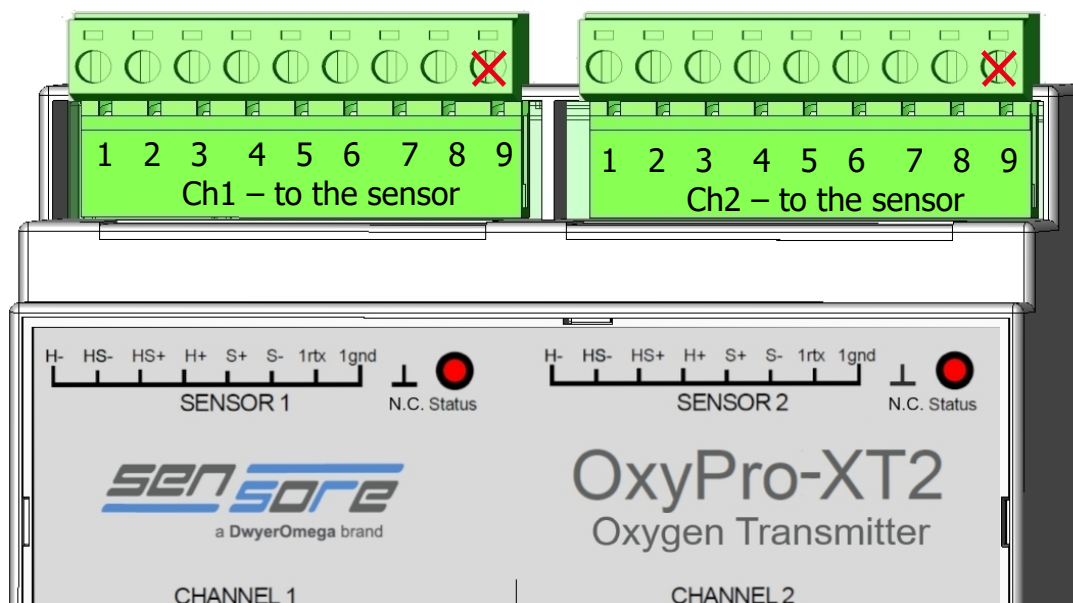

X = No connections in these terminals

Figure 5. Sensor Side Connections

POs	Function	Information
1	Sensor H-	To be connected to sensor cabling
2	Sensor HS-	To be connected to sensor cabling
3	Sensor HS+	To be connected to sensor cabling
4	Sensor H+	To be connected to sensor cabling
5	Sensor S-	To be connected to sensor cabling
6	Sensor S-	To be connected to sensor cabling
7	1rtx (1-Wire-EEPROM)	To be connected to sensor cabling
8	1gnd (1-Wire-GND)	To be connected to sensor cabling
9	N.C.	Not connected (reserved for alternative grounding)


3.3 Sensor Connection

3.3.1 Connection via M12 cable extension (maximum 3 m)

The M12 extension cables must meet the following requirements:

- Sensor direction: M12 female, 8-pin, A-coding
- Cable: AWG24/0.25 mm², shielded, maximum length 3 m
- Direction electronics: open end of cable for screw terminal connection, or a fitting 9-pol socket

- Correct mapping of the M12 pins with electronic terminal positions:

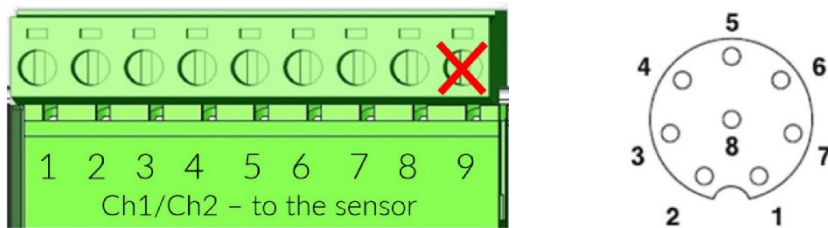

Sensor Side		DIN 47100 Color Code	M12 Pin No.
POs	Function		
6	Sensor S-	White	1
5	Sensor S-	Brown	2
8	1gnd	Green	3
7	1rtx	Yellow	4
2	Sensor HS-	Grey	5
3	Sensor HS+	Pink	6
1	Sensor H-	Blue	7
4	Sensor H+	Red	8

NOTE: The Color code may differ from DIN 47100.

3.4 Route Cables and Shielding Grounding

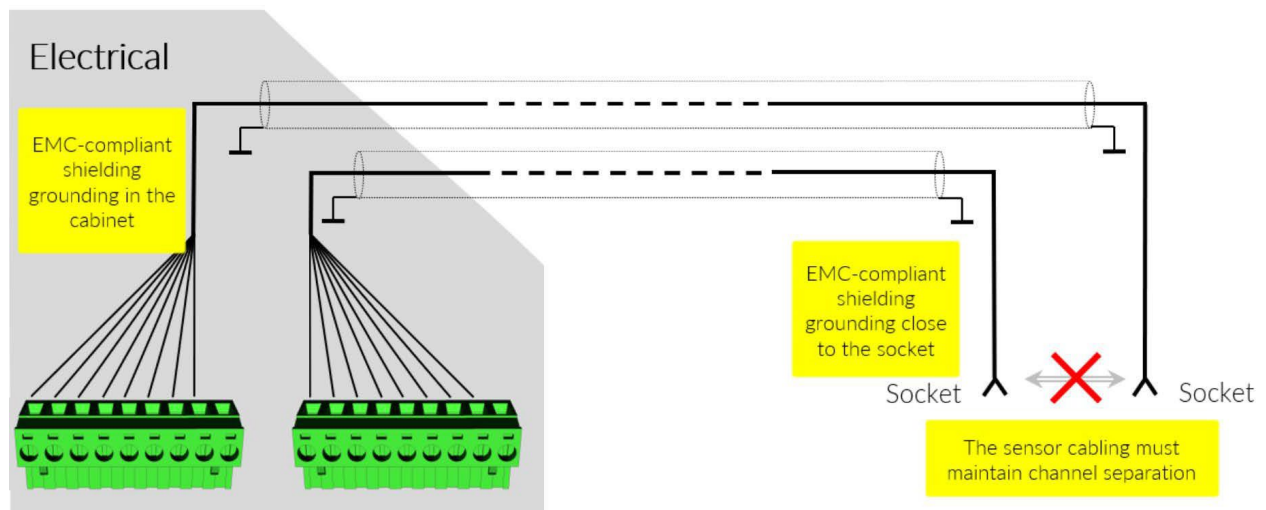


Figure 6. Shielding Grounding

4 Commissioning

A basic function test should be carried out before using the OxyPro-XT (see 5.2).

4.1 Initial Power-up

- The system will power-up as soon as the supply voltage is connected.
- After initial power-up, the basic function test (see 5.2) should be carried out

4.2 Power-up after Maintenance

- After power-up following maintenance, the basic function test (see 5.2) should be carried out

4.3 Decommissioning

- The system can be safely powered-down by disconnecting the supply voltage.

4.4 Recommissioning

- The system will restart as soon as the supply voltage is connected.
- For recommissioning after a malfunction, please refer to section 8.2.

4.5 System Behavior During Commissioning

Commissioning In dry air (20.9%) with a 25 % sensor						
System states	Duration (secs)	Analog output		Digital output / LED		
		4...20 mA	0...5 V	state	O2norm	LED
Contact Check	< 1	-	-	2	-	-
Heating up	~ 30	~ 19.15 mA	~ 5.00V	4	na	Flashing
Stabilizing	~ 30	~ 19.15 mA	~ 5.00V	4	na	Flashing
Measuring O2	Continuous	~ 17.38 mA (~ 20.9 %)	~4.18 V (~ 20.9 %)	5	~836 (~ 20.9 %)	On

5 Maintenance

5.1 Inspect Your Sensors/Sensor Cleaning

The sinter caps of the sensor must be checked for visible contamination.

The sensors must only be cleaned mechanically (brushing), no chemical cleaning agents or water may be used for cleaning.

5.2 Inspect Your OxyPro-XT – Basic Function Test

The basic function test is a plausibility check of the complete system by exposing the sensor to air.

- 25% and 96% sensor are supposed to show a value around 20.7 vol % O₂
- Sensors with lower ranges are supposed to show full-scale reading. Remark: lower range sensors should not be permanently exposed to air (20.7 vol % O₂) as this will accelerate sensor aging. Short-time exposure (hours) to air to check signal plausibility is ok.

5.3 Process Measurement Accuracy

Hardware self-monitoring and basic function test (5.2) will detect significant fault conditions of the system. Further measures may be required to monitor process accuracy, e.g. expose the sensor to reference gas concentrations to verify the process measurement accuracy.

6 Repairs and Replacements

6.1 Replace the Sensor

The typical sensor replacement interval depends on several external factors:

- Application conditions, especially:
 - Contamination load and type (e.g.: VOCs, some chemicals/gases)
 - Mechanical and thermal stress (vibrations, ambient temperature)
 - Other environmental factors (e.g. operating pressure, condensation risks)
- Use case:
 - Sensor operating parameters
 - Operating hours (e.g., continuous 24/7 vs. intermittent use)
- Customer-specific requirements:
 - Desired accuracy at a given O₂ level, sensors should be replaced either at the end of the maximum service life (5 years) or if they are defective.

Procedure for sensor replacement:

- Before replacing the sensor, the OxyPro-XT must be powered down.
- If the sensor is replaced during operation, the transmitter may switch to a fault mode for approximately 60 seconds. If faults are triggered repeatedly over a short period of time, the system may switch into a permanent fault mode. This can be resolved by a power cycle.
- Ensure general practice ESD precautions are adhered to while changing the sensor.
- During sensor replacement ensure that the new sensor is:
 - Sealed to the process chamber
 - Relocked at its connector.
- After the sensor has been replaced, the transmitter can be powered up.
- Once replaced, carry out a function test of the system (see 5.2).



6.2 Replace the OxyPro-XT transmitter

If the transmitter must be replaced, the sensor(s) do not need to be replaced if they are still performing well.

After replacing the transmitter, a function test should be carried out (see 5.2).

6.3 Installation Changes

- If the transmitter's wiring is altered during a repair, a basic function test (see 5.2) must be carried out afterwards.
- If transmitter components (e.g. power supply) are replaced, a basic function test (see 5.2) must be carried out afterwards.

7 Disposal and Recycling

Dismantling the OxyPro-XT must be carried out when it is powered off.

The system must be disposed of appropriately, and sensors must be disposed of as electronic waste.

8 Troubleshooting

If the system detects a fault condition, it will initiate the following:

- Open relay contacts
- Switch into a failure mode, indicated with flashing LEDs and 19 mA analog output, see also section 9.5
- After 1 minute in failure mode, the system will initiate an automatic restart
- Following repeated automatic restarts, the system will enter a permanent error state, see section 9.5

To recover from a permanent error state, see section 8.2

8.1 Error Codes

No.	Error State	Description	Troubleshooting/Cause
0	No error		
1	Channel	Fault detected on the other channel	Will not apply to OxyPro-XT (only 1 channel)
2	Heating	Failure during the heat-up phase	Occasional errors are automatically resolved by restarting the heating process For persistent heat-up errors, check sensor wiring or replace sensor
3	Heater open circuit	Fault with sensor heater	Check sensor wiring or replace sensor
4	Heater short circuit	Fault with sensor heater	Check sensor wiring or replace sensor
5	Heater control	Incorrect sensor temperature	Check sensor wiring or replace sensor
6	Sensor cell	Implausible sensor current/voltage	Check sensor wiring or replace sensor
7	24 V	Incorrect or faulty supply voltage	Check external supply voltage
8	3V3	Internal voltage fault	Check the external supply voltage. If persistent or repetitive, replace the transmitter
9	1V1		
10	Overtemperature	Over-temperature of electronics	Check the temperature near the transmitter. If persistent or repetitive, replace the transmitter
11	Watchdog	Internal electronics monitoring errors	If persistent or repetitive, replace the transmitter.
12	Relay		
13	Reserved		
14	Error on Uout	Faulty connection of Uout	Check Uout terminal and connection
15	EE Error External	Fault with the EEPROM of the sensor	Check sensor wiring or replace sensor
16	EE Error Internal	Fault at the sensor EEPROM	Invalid EEPROM data. If parameter data is corrupted, contact SENSORE.
17	Flash	Self-monitoring error detection	If persistent or repetitive, replace the transmitter.
18	RAM		
19	System		
20	Parameter	Invalid sensor parameters	Sensor memory error, replace sensor
21	Watchdog	Critical error in the SW sequence	If persistent or repetitive, replace the transmitter.

8.2 Recovering from (Permanent) Fault Conditions

8.2.1 Via RS232/Modbus

To restart switch to programming mode then initiate measurement mode, see 9.4.3

8.2.2 Disconnect (and reconnect) Power Supply

- Disconnect the power supply for at least 5 seconds.
- Reconnecting the power supply.

8.2.3 Disconnect (and reconnect) Sensors

Disconnecting/ and reconnecting the sensors will also restart the system without requiring a power cycle. Reconnecting a sensor when the system is powered-up may trigger a new fault condition, in this case it is important to wait approximately 60 seconds until the system recovers automatically.

8.3 Interference with O₂ Measurement

The OxyPro-XT is designed for measurement in O₂/N₂ or O₂/Ar atmospheres, i.e. it is assumed that other gases only occur in trace amounts (< 1000 ppm).

8.3.1 Temporary Impairment of O₂ Measurement

- Rapid pressure fluctuations can lead to a short-term disturbance of the O₂ measurement, such influences can be reduced by averaging the output measured analog signal over time
- Operating below the specified measuring range increases the cross-sensitivity to oxygen containing gases such as H₂O (water vapor) or CO₂, which leads to an increase in the O₂ measurement signal.
- Traces of flammable gases can lead to a reduction in the O₂ measurement signal if present in a high enough concentration.

8.3.2 Permanent Impairment of O₂ Measurement

- When the Pt-ZrO₂ electrode is damaged by chemical substances, the sensor aging may accelerate, leading to permanent reduction in the O₂ measurement signal.
 - Volatile silicone compounds (silanes), e.g. generated by the out-gassing of silicone seals, are particularly harmful to the sensors' measurement performance
- When used in chemically aggressive environments, a damaged glass seal of the sensor cell can cause leakages, leading to a permanent increase in the O₂ measurement signal.
 - e.g. environments that try to reduce O₂ by chemical means.
- Condensing environments can lead to destruction of the sensor cell.
- The function test is used to detect a permanent impairment (see 5.2).

9 RS485 Modbus Interface

9.1 RS485 Parameters

Baud Rate	19200
Start Bits	1
Data Bits	8
Stop Bits	1
Parity	None

9.2 Modbus Functions

To limit the impact on the measurement performance a maximum of one addressed transmission per second is recommended, see also table below for the recommended multiple register access.

	Read Only Register	Read/write Registers		
	fct 0x04 (Read)	fct 0x03 (Read)	fct 0x06 (Write)	fct 0x16 (Write)
O2 Measurement	Max. 4 registers	Max. 4 registers	not recommended	not recommended
PRG Mode	Multiple registers	Multiple registers	1 register	Multiple registers

General remarks regarding writing to the OxyPro-XT via Modbus:



- Writing via MODBUS could potentially corrupt the EEPROM data of the OxyPro-XT. So, writing commands should be only used during the initial setup or maintenance of the OxyPro-XT.
- The writing should be limited to the registers documented in this manual.
- Other register values are protected by a checksum, i.e. in the event of inadmissible changes, the system will switch to error mode. Please contact SENSORE in such a case to restore the EEPROM data integrity.

9.3 Modbus Communication Examples

9.3.1 Readout of the status register via Modbus function 0x04 (Read Only register)

Hexadecimal data packet sent:

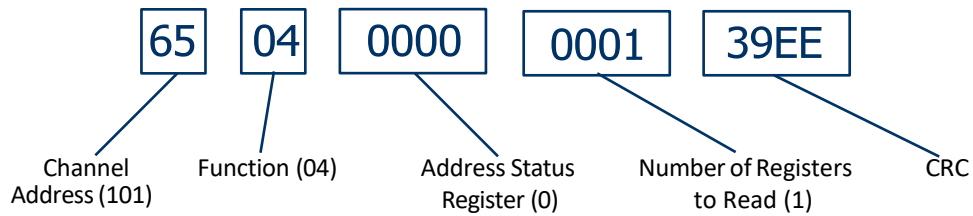


Figure 7. Hexadecimal data packet sent

CRC Calculation:

- For the above hexadecimal data sequence 0x650400000001
 - Seed value 0xFFFF
 - Polynomial 0x8005
- Provides 0xEE39 => Modbus protocol LSB/MSB => 0x39EE

Received hexadecimal data packet:

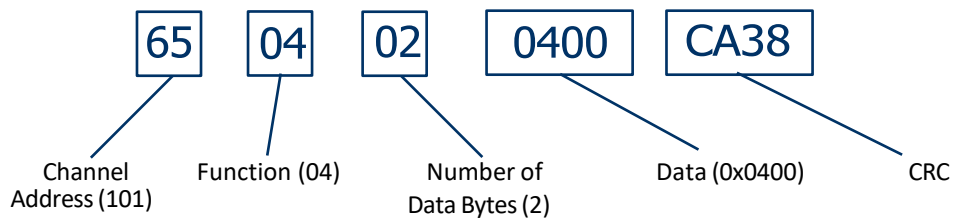


Figure 8. Received hexadecimal data packet via Modbus function 0x04

Modbus data is based on the “big endian” representation i.e. 0400 corresponds to 0x0400:

- MSB 0x04 => b 0000 0100 => measurement mode active; relay contact open
- LSB 0x00 => no error

9.3.2 Readout of status and O₂ level via Modbus function 04 (Read Only register)

Hexadecimal data packet sent:

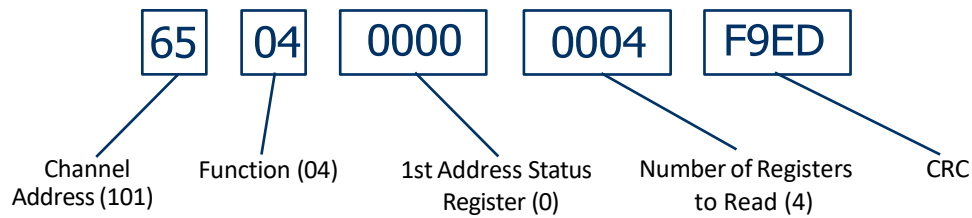


Figure 9. Hexadecimal data packet sent via Modbus function 04 (ppm)

Received hexadecimal data packet:

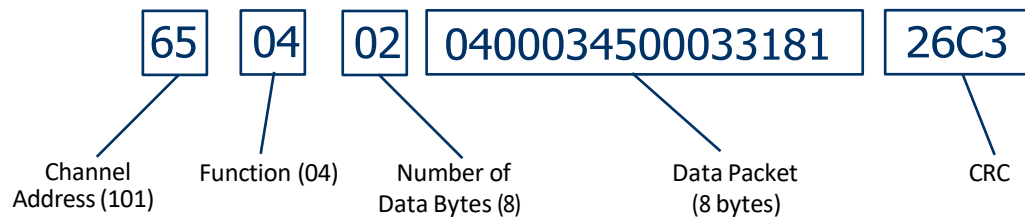


Figure 10. Received hexadecimal data packet

Breakdown of the data package:

- 2-byte status register: 0x0400 see 9.5
- 2-byte O₂ normalized: 0x0345 => 837 Dec.
 - In this example, normalized to 25 % O₂, i.e. $837/1000 \cdot 25\% \text{ O}_2 \Rightarrow 20.925\% \text{ O}_2$
- 4-byte O₂ and ppm: 0x00033181 => 209.281 ppm O₂

9.4 Modbus Register Overview

The following tables provide an overview of the most important registers

9.4.1 Modbus function code 0x04 (useful in measurement mode) “Read” register

Modbus Address	Data Type	Description
0x0000	unsigned int16	Status register LSB (least significant bits 1...8) 0 ... no error, >0 ... error code when the error state is active (see section 8.1)
		Status register MSB (most significant bits 9...16)
		Status Flags (see section 9.5)
0x0002	unsigned int16	O ₂ value (digital) normalized
0x0004-6	unsigned int32	O ₂ value absolute (in ppm O ₂)

Modbus Address	Data Type	Description
0x0008	unsigned int16	Current sensor current (in 0.1 uA)
0x000A	unsigned int16	Current sensor temperature (in °C)
0x000C	unsigned int16	Current sensor voltage (in mV)
0x000E	unsigned int16	Current heater voltage (in mV)
0x0010	unsigned int16	Current heater current (in 0.1 mA)
0x0012	unsigned int16	Adjusted cold heater resistance
0x0014	unsigned int16	Current heater resistance during operation
0x0016	unsigned int16	Digital system states (0...7) (see 0)
0x0022	unsigned int16	Last error code encountered since powering on
0x007C	unsigned int16	FW Rev (120 => v1.20)
0x007E	unsigned int16	Reading this address will switch to Programming Mode (PRG) from Measuring Mode

9.4.2 Modbus function code 0x03/0x06 (usable in PRG mode) “Write”/“Read” tabs

Modbus Address	Data Type	Description
0x1012	unsigned int16	Registry contains Modbus address

9.4.3 Modbus function code 0x06 “Write” register to execute commands

Modbus Address	Data Type	Description
0x0102	unsigned int16	Switch to programming mode
0x0104	unsigned int16	Initiation of measurement mode (from programming mode)

To quit a permanent error mode, apply the following command sequence:

- Switch to programming mode (0x0102), writing any value into the register will trigger the command
- Switching to measurement mode (0x0104), writing any value into the register will trigger the command

9.4.4 Modbus function code 0x06 “Write” registers for customized threshold setting

Modbus Address	Data Type	Description
0x1322	signed int16	Threshold value normalized (1000 ... full scale) negative sign ... open when exceeding positive sign ... open when fall below
0x1324	unsigned int16	optional 2nd threshold value for range switching, otherwise 0
0x1326	unsigned int16	Hysteresis value (also scaled with 1000 ... full scale)
0x1328	signed int16	Checksum values [0x1322] + [0x1324] + [0x1326]

Preset value of registers 0x1322 – 0x1328 is 0, which will deactivate the customized threshold settings. If the checksum in 0x1328 is incorrect the settings will be ignored.

The calculations for the threshold and hysteresis are based on the normalized digital output; see section 2.4. The normalization value is 1000, scaled over the usable digital range; refer to the table in section 2.2. See the examples below for how the calculation is performed. Please contact SENSORE if further assistance is needed.

Example 1: 25 % sensor, contacts should open when 2 % O₂ is exceeded, hysteresis 0.2 % O₂:

usable digital range is 25 % ... 1000	=> 2 %	... 80
(-) to open when exceeded	=> -80	to be written into 0x1322
no 2 nd threshold value needed	=> 0	to be written into 0x1324
hysteresis 0.2% ... 8; hysteresis is always a positive value	=> 8	to be written into 0x1326
Checksum is -80 + 0 + 8 = 72	=> 72	to be written into 0x1328

Result: Relay contacts will open at > 2 % O₂ and close at < 1.8 % O₂

Example 2: 1000 ppm sensor, contacts should open when O₂ falls below 600ppm, hysteresis 30ppm O₂:

usable digital range is 1200ppm ... 1000	=> 600ppm	... 500
(+) to open when fall below	=> +500	to be written into 0x1322
no 2 nd threshold value needed	=> 0	to be written into 0x1324
hysteresis 30ppm ... 25; hysteresis is always a positive value	=> 25	to be written into 0x1326
Checksum is 500 + 0 + 25 = 525	=> 525	to be written into 0x1328

Result: Relay contacts will open at < 600ppm O₂ and close at > 630ppm O₂

9.4.5 Modbus function code 0x06 "Write" registers for customized 19-20mA error output

Modbus Address	Data Type	Description
0x132A	unsigned int16	standard value 0 (customization disabled, setting is defined by sensor) customized value 1900...2000 (19...20 mA)

Usually, values > 19 mA are used to display special states and error conditions. This setting is stored in the memory chip of the Smart Sensor.

If the full 4...20 mA range should be used for the analog sensor signal, it is possible to shift the error indication range to > 20 mA, by writing 2000 in the register 0x132A. It is necessary to restart the OxyPro-XT, so that the change will go into effect.

9.5 Digital Status Register 16Bit (Modbus Register 0x0000)

- Bits 1-8: 8-bit integer: 0 ... no error or error code (see section 8.1).
- Bits 9-16: bitwise flags: 1 ... if state/phase is active or 0... if state/phase is inactive

The relay status flag will be 1 if the relay is closed, or 0 if it is open.

Bit 16	Bit 15	Bit 14	Bit 13	Bit 12	Bit 11	Bit 10	Bit 9
Permanent error state	Error over-temperature	Contact check	Not used by XT	Heat-up mode	Measuring mode	Relay status flag	Not used by XT

9.6 Digital System States (Modbus Register 0x0016)

Number	Description of System State
0	Initializing
1	Not in use (customized option)
2	Contact check (and import of sensor EEPROM data)
3	Not in use (customized option)
4	Heating mode (and stabilization of the sensor signal)
5	Measuring mode
6	Programming mode
7	Failure mode (temporary or permanent)

10 Appendices

Appendix A - Technical Specifications

Sensors		Zirconia (ZR)					
Available measurement ranges		O2 concentration in volumetric % or ppm					
Nominal sensor range*	1000 ppm	1.00 %	2.00 %	5 %	25 %	40.0 %	96.0 %
Analog full scale (19mA)	1125 ppm	1.17 %	2.35 %	5.86 %	23.5 %	46.9 %	93.8 %
Usable digital range (RS 485)	1200 ppm	1.25 %	2.5 %	6.25 %	25 %	50 %	100 %
Typical Accuracy	20 ppm	100 ppm	200 ppm	500 ppm	0.25 %	0.40 %	1.0 %
Output Resolution (4...19 mA)	< 1 ppm	< 10 ppm	< 20 ppm	< 50 ppm	< 0.025 %	<0.04 %	<0.1 %
Lower Detection Limit	10 ppm	100 ppm	100 ppm	500 ppm	0.1 %	0.2 %	1.0 %
		*Nominal sensor range is the specified maximal O2 concentration, overrange operation should be avoided					
General sensor specification							
Maximum flow velocity	6 m/s (19.7 ft/s)						
Pressure Range (Maximum Altitude)	700...1300 mbara (10...19 psia) (3000 m)						
Maximum Safe Pressure	1500 mbarg (21 psig)						
Response Time (T90)	depend on selected sensor housing (fastest option D0 < 5 seconds)						
Operating Temperature Range (Sensor head)	depend on sensor cable configuration, in any case +10...+100 °C (+50...+212 °F)						
Operating Temperature Range (Sensor plug)	+10...+75 °C (+50...+165 °F)						
Life Expectancy (application dependent)	Up to 5 years						
Humidity (with normal use)	0...90 %rh @ 40 °C (104 °F) non-condensing						
Available Housing configurations	D0 (M16 x 1.5 male), D2 (alu, M16 x 1.5 male), D3 (alu, M18 x 1.5 male), B1 (TO8 + flange)						
Shelf Life	Unlimited						
Calibration Interval	No calibration required. Calibration data stored in smart sensor.						
Analyzer (Monitor)							
Electrical							
Output Signal	4...20 mA (19...20 mA Error or Special Condition) 19 mA = analog full scale						
Digital Communications	RS485 / Modbus RTU						
Relay Contact Output	to switch 24Vdc / 100mA, controlled by an O2-alarm-level (programmable via RS485)						
Electrical Interface	8-pin M12 on sensor, extension cable from sensor plug to screw terminal on monitor						
Operating Temperature Range (Monitor)	+10...+50 °C (+50...+122 °F)						
Power Supply	24 V DC ± 10%						
Maximum Power Consumption	6 W or 0.25 A						
Mechanical							
Ingress Protection	IP40 (Monitor), IP66 (Sensor plug)						
Housing Material	PC (UL 94 V-0)						
Mounting	DIN rail						
Sensor Cable Length	50 cm (19.6”) with 8 pin M12 connector						
Extension Cable Length	1 m (3.28 ft) or 3 m (9.8 ft)						
Compliance							
CE: According to EU Machinery Directive EN ISO13849-1 Performance Level a / non-SIL applications only, also compliant with EN 61010-1							


Appendix B - Technical Drawings (mm)

The OxyPro-XT uses DIN-Rail housings based on standard width units 1TE=18mm

OxyPro-XT (1channel) nominal width 3TE (54mm)

OxyPro-XT2 (2channel) nominal width 6TE (108mm)

The actual width is slightly smaller, see the drawing of the OxyPro-XT below

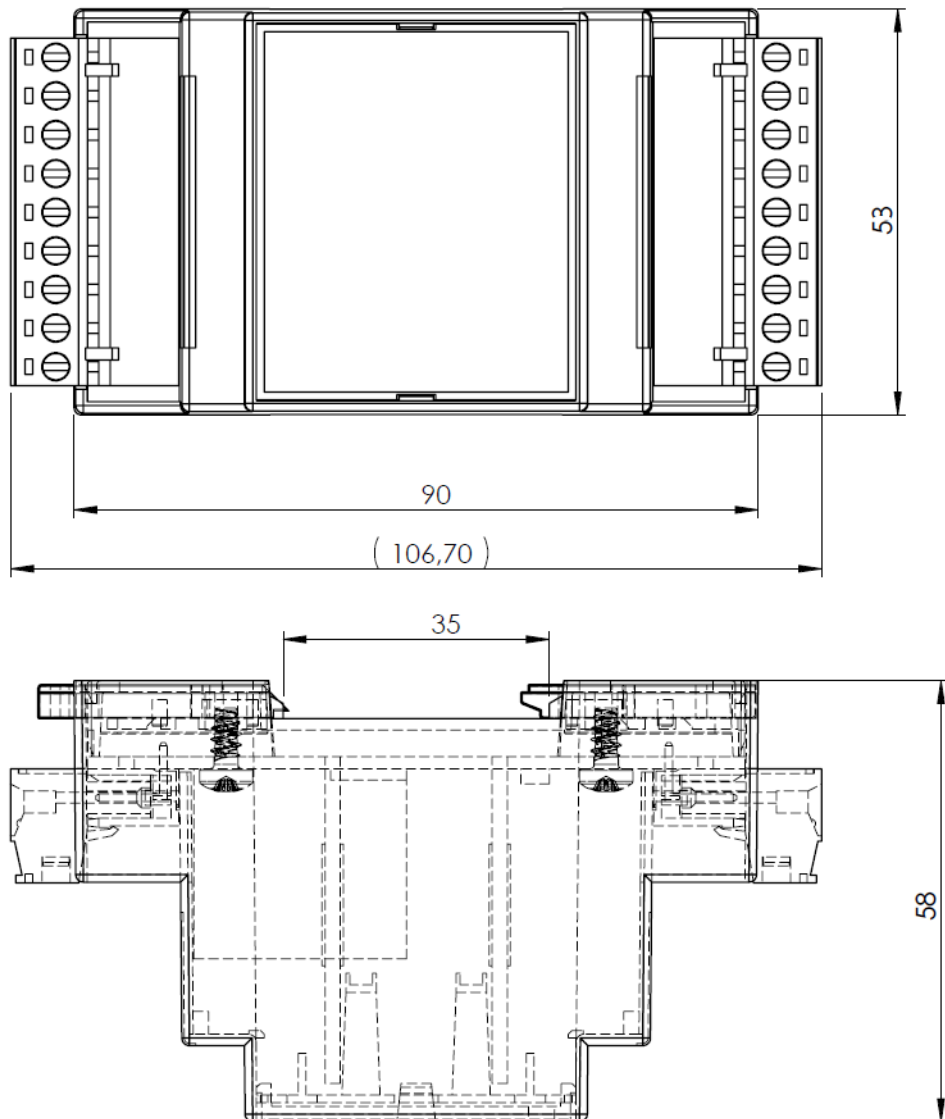

Appendix C - Quality, Recycling, and Warranty Information

SENSORE Electronic GmbH. is part of the DwyerOmega Group. and complies with applicable national and international standards and directives.

The following regulations have been considered:

- CE
- UKCA
- REACH (Registration, Evaluation, Authorization, and Restriction of Chemicals)
- Recycling policy
- RoHS (Restriction of Hazardous Substances in electrical and electronic equipment)
- WEEE (Waste Electrical and Electronic Equipment recycling)

This page is intentionally blank.



Sensore Electronic GmbH Aufeldgasse 37-39 A-3400 Klosterneuburg, Austria, Tel: +43 2243 450-0
www.sensore-electronic.com email: sensors@dwyeromega.com